

HENSO
for better life
Blood Collection
Collecte de sang

for better life



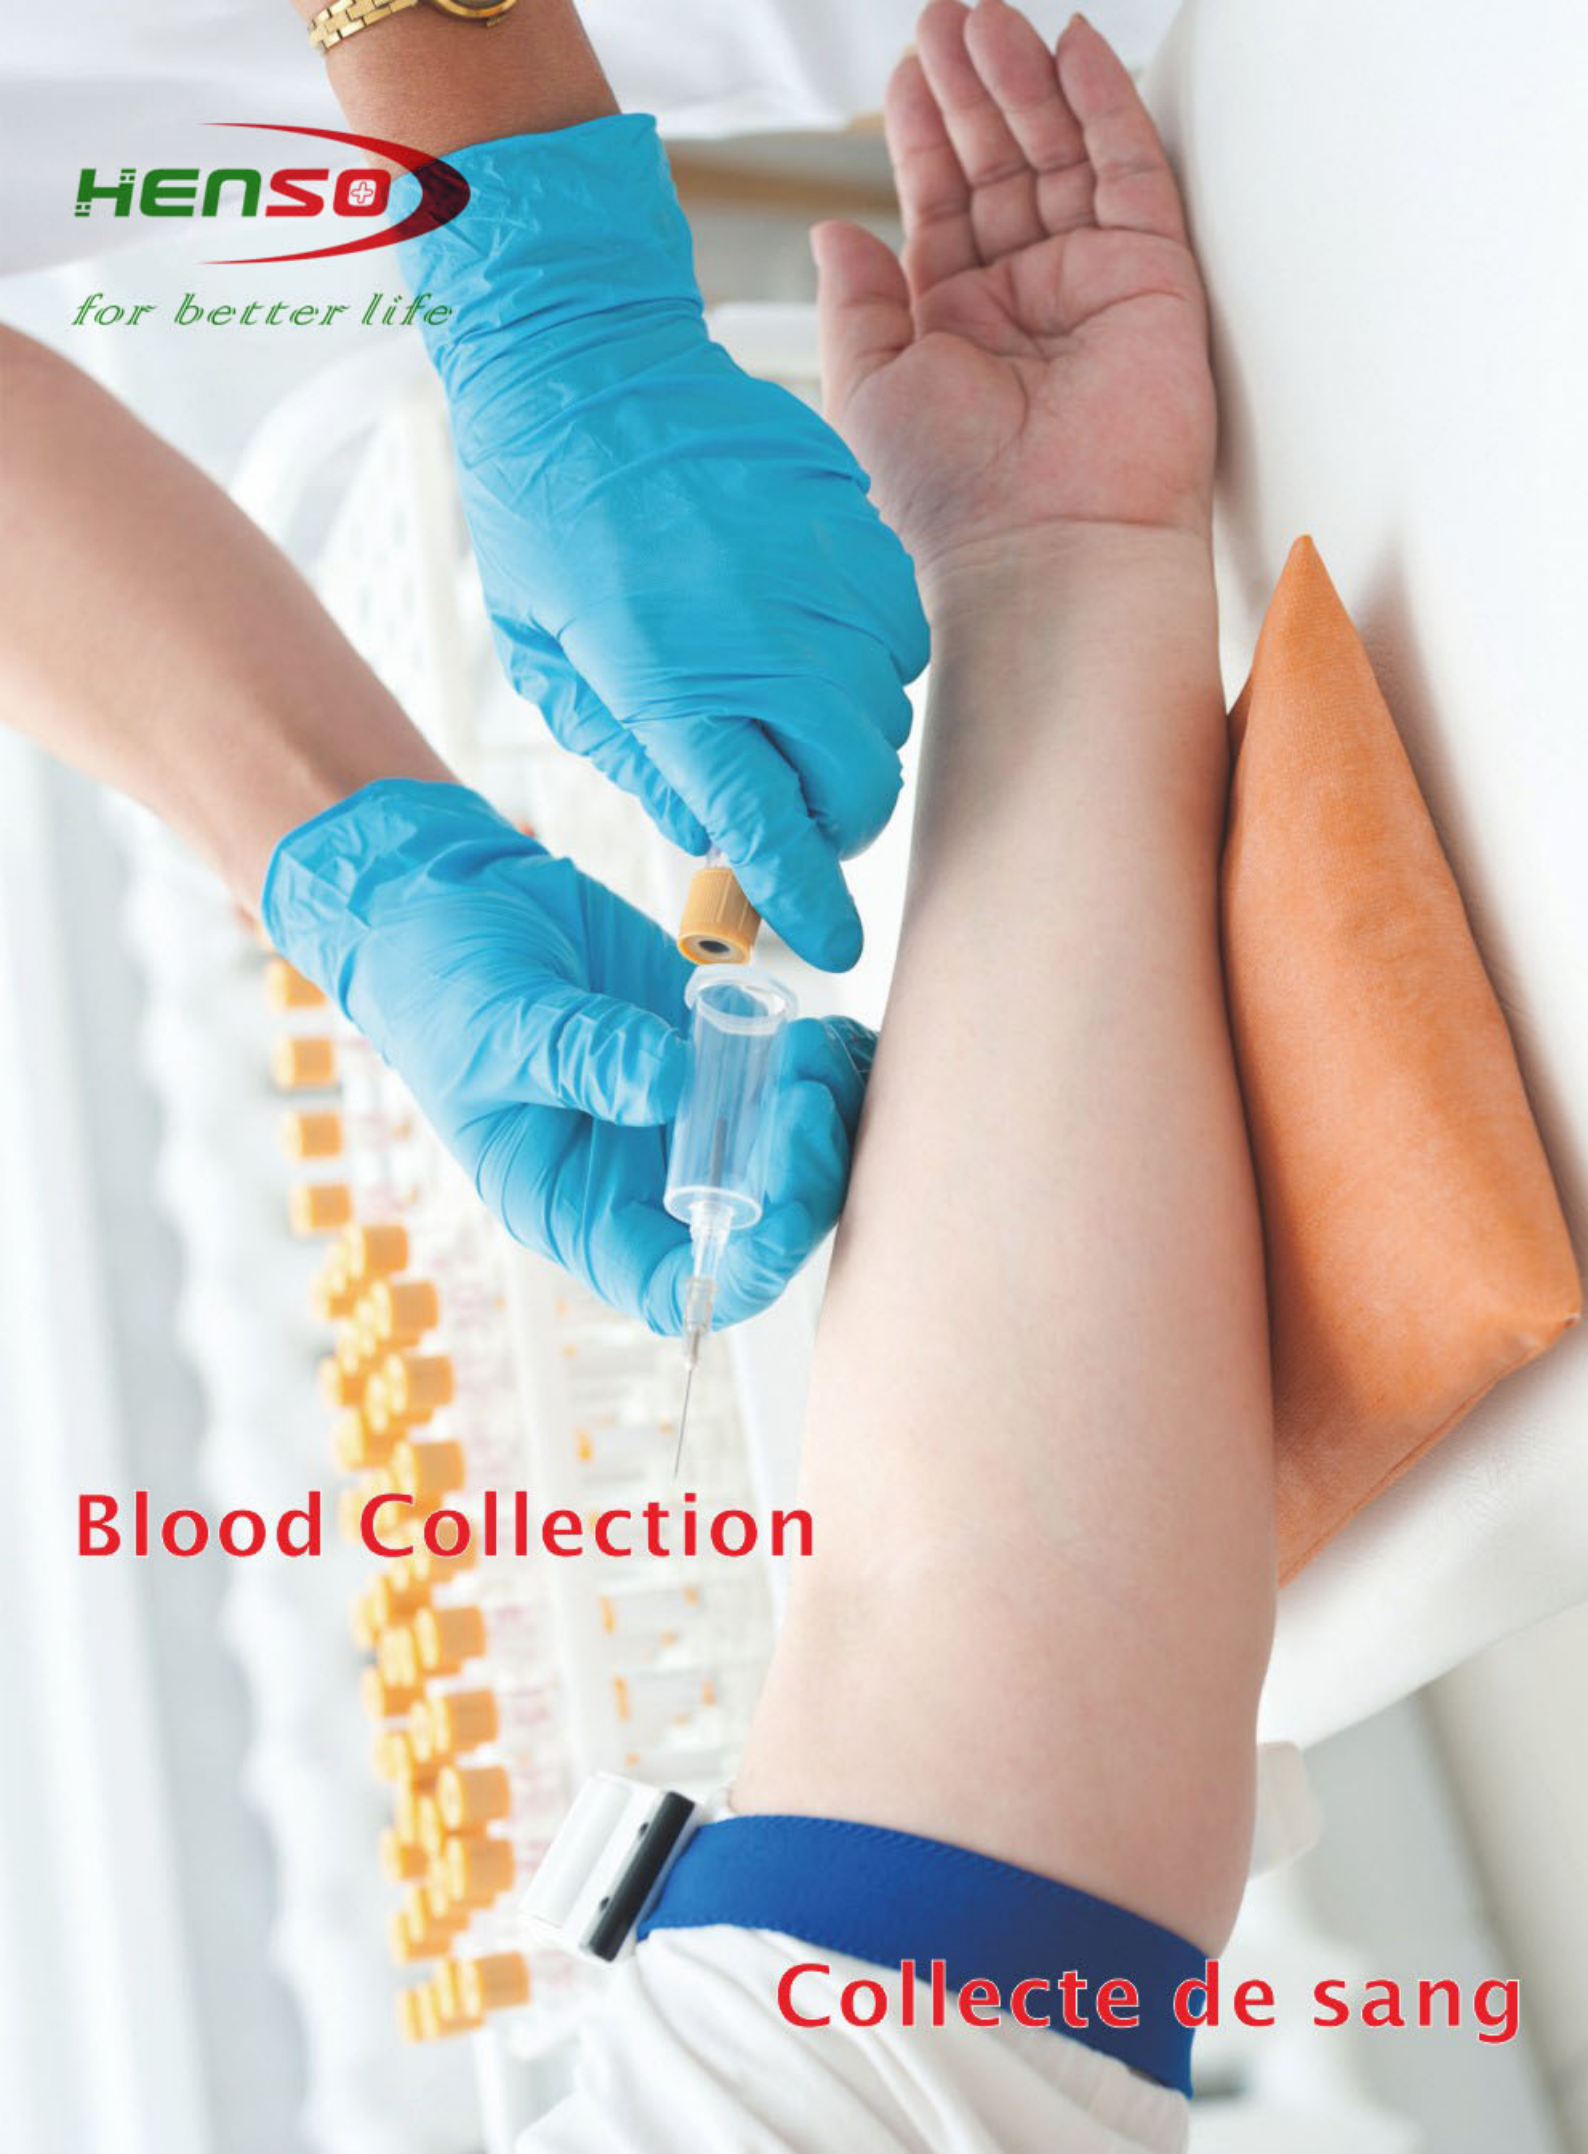

OUR MISSION:

Since the moment of establish, Henso are committed to offer one-stop solution for medical supplies, to reduce medical expense by supply reliable products with affordable cost. We are efforts for human's better life.

GOOD MANUFACTURING PRACTICES:

Our Manufacturing plant conforms to GMP, a WHO proprietary benchmark. This standard is evident in the physical ambience of our plant, the air and water quality, manufacturing technology, packaging and the sterilization process. Ambience: Special micro and HEPA filter at all air handling units ensure minimal contamination in all manufacturing areas. Micro organism and particle concentration levels are carefully monitored by the micro-biological lab to keep these levels within safe limits. Employees undergo periodic medical checkup to maintain high standards of health and hygiene. All clean rooms are provided with a three step change room and air showers at the entrance to ensure a dust-free environment.

PURSUIT ZERO DEFECT QUALITY:

Manufacture zero-defect products is our goal of quality. We have built a series online and manual quality control measures into each stage of raw material procurement, manufacturing and packing cycle. Our Quality Control standards conform to ISO 13485:2012 and European Medical Device Directive 93/42/EEC Annex V. We also registered with US FDA. As a result, our products have been authorized to lable prestigious CE mark.

PACKING AND STERILIZATION:

Our products are packed by most modern packaging machines, to ensure minimal risk of contamination or damage during transportation. We use Ethylene Oxide to sterilize the product, as per ISO 11135/EN 550 standards, each batch were release after strict inspection.



Vacuum Blood Collection Tube (Plain Tube)
Tube à prélèvement de sang Vacuum (Tube plaine)

HSE0501

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: No Additive
- Color code: Red top
- Test Specimen: Serum
- Tube Size: 13x75mm, 13x100mm, 16x100mm
- Vacuum Draw Volume: 1ml-10ml
- Max. Vacuum Degree Tolerance: ±10%

Vacuum Blood Collection Tube (Serum Tube)
Tube à prélèvement de sang Vacuum (Tube Sérum)

HSE0502

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: Clot Activator
- Color code: Red top
- Test Specimen: Serum
- Tube Size: 13x75mm, 13x100mm, 16x100mm
- Vacuum Draw Volume: 1ml-10ml
- Max. Vacuum Degree Tolerance: ±10%





Vacuum Blood Collection Tube (EDTA Tube)
Tube à prélèvement de sang Vacuum (Tube EDTA)

HSE0503

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: K2 EDTA or K3 EDTA
- Color code: Lavender top
- Test Specimen: Whole Blood
- Tube Size: 13x75mm, 13x100mm, 16x100mm
- Vacuum Draw Volume: 1ml-10ml
- Max. Vacuum Degree Tolerance: ±10%



Vacuum Blood Collection Tube (SST Tube)
Tube à prélèvement de sang Vacuum (Tube SST)

HSE0504

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: Gel & Clot Activator
- Color code: Yellow top
- Test Specimen: Serum
- Tube Size: 13x75mm, 13x100mm, 16x100mm
- Vacuum Draw Volume: 1ml-9ml
- Max. Vacuum Degree Tolerance: ±10%

Vacuum Blood Collection Tube (Heparin Tube)
Tube à prélèvement de sang Vacuum (Tube héparine)

HSE0505

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: Lithium Heparin or Sodium Heparin
- Color code: Green top
- Test Specimen: Plasma
- Tube Size: 13x75mm, 13x100mm, 16x100mm
- Vacuum Draw Volume: 1ml-9ml
- Max. Vacuum Degree Tolerance: ±10%





Vacuum Blood Collection Tube (Glucose Tube)
Tube à prélèvement de sang Vacuum (Tube glucose)

HSE0506

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: Sodium Fluoride+Potassium Oxalate
- Color code: Grey top
- Test Specimen: Plasma
- Tube Size: 13x75mm, 13x100mm
- Vacuum Draw Volume: 2ml-6ml
- Max. Vacuum Degree Tolerance: ±10%



Vacuum Blood Collection Tube (PT Tube)
Tube à prélèvement de sang Vacuum (Tube PT)

HSE0507

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: 3.2% Sodium Citrate (1:9)
- Color code: Blue top
- Test Specimen: Plasma / Whole Blood
- Tube Size: 13x75mm, 13x100mm
- Vacuum Draw Volume: 1.8ml, 2.7ml, 3.6ml, 4.5ml
- Max. Vacuum Degree Tolerance: ±5%

Vacuum Blood Collection Tube (ESR Tube)
Tube à prélèvement de sang Vacuum (Tube ESR)

HSE0508

- Material: Glass or PET tube, PVC cap, rubber stopper
- Additive: 3.8% Sodium Citrate (1:4)
- Color code: Black top
- Test Specimen: Whole Blood
- Tube Size: 13x75mm, 13x100mm, 8x120mm
- Draw Volume: 1.28ml, 1.6ml, 2.4ml, 3.2ml, 4.0ml
- Max. Vacuum Degree Tolerance: ±5%





Non-Vacuum Blood Collection Tubes
Tube à prélèvement de sang non vide

HSE0509

- Structure: PP tube + PP insert cap
- Type: Plain Tube, Serum Tube, EDTA Tube, SST Tube, Heparin Tube, ESR Tube, PT Tube, Glucose Tube
- Color coded top for easy identification
- Test Specimen: Serum / Plasma / Whole Blood
- Tube Size: 13x75mm, 13x100mm
- Volume: 1ml-6ml



Micro Blood Collection Tube (Screw Cap)
Tube à prélèvement de sang micro (bouchon à vis)

HSE0510

- Made from medical grade PP
- Types: No Additive, Clot Activator, EDTA K2/K3, Gel & Clot Activator, Lithium Heparin
- Color coded screw cap for easy identification
- Tube Size: 8x45mm
- Volume: 0.25-0.5ml (250-500ul)
- Suitable for small children and geriatriatric patient

Micro Blood Collection Tube (Rubber Stopper)
Tube à prélèvement de sang micro (bouchon de caoutchouc)

HSE0511

- PP tube + Cross-cut rubber stopper
- Types: No Additive, Clot Activator, EDTA K2/K3, Gel & Clot Activator, Lithium Heparin, Glucose, 3.2% Sodium Citrate, 3.8% Sodium Citrate
- Color coded cap for easy identification
- Volume: 0.2-0.5ml (200-500ul)
- Suitable for small children and geriatriatric patient





Micro-Hematocrit Capillary Tube
Tube micro hématocrite

HSE0512

- Medical grade clear glass
- Types: Sodium-heparinized 80IU/mL (Red top) Non-heparinized (Blue top)
- Diameters: I.D.: 1.1-1.2mm, O.D.: 1.5-1.6mm
- Tube Length 75mm
- Supplied inside cylindrical box with a cap
- Barrel of 100, Box of 10 Barrels



Multi-Sample Blood Collection Needle
Aiguille de prélèvement multiples

HSE0513


- Multi-sample type with luer adapter
- Latex free, non-toxic, non-pyrogenic
- Sharp, smooth edges make painless puncture
- Needle Gauge: 18G, 20G, 21G, 22G, 23G
- Needle Length: 1", 1 1/4", 1 1/2"
- Color coded plastic cover for gauge identification
- Sterile EO, for single use only

Flashback Blood Collection Needle
Aiguille de prélèvement Flashback

HSE0514

- Flashback chamber as a blood view window
- Unique design for blood flow
- Special cut needle tip make comfort penetration
- Needle Gauge: 20G, 21G, 22G, 23G
- Needle Length: 3/4", 1", 1 1/4", 1 1/2"
- Color coded plastic cover for gauge identification
- Sterile EO, for single use only



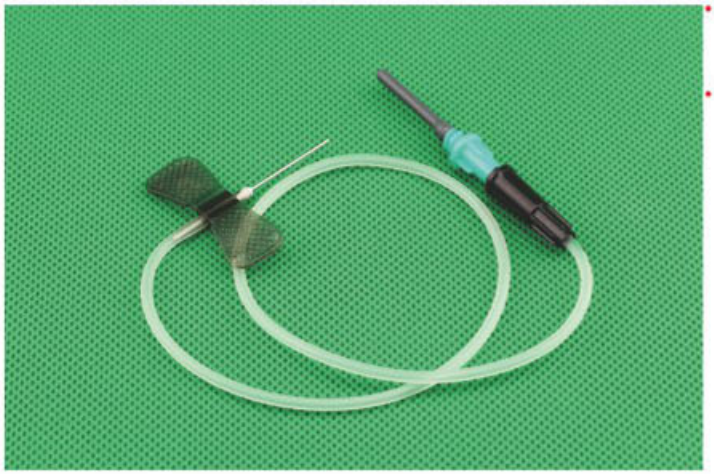

Butterfly Blood Collection Needle
Microperfuseurs avec adaptateur pour prélévement

HSE0515

- Butterfly type with detachable luer adapter
- Transparent tube for easy observe of blood flow
- Sharp, smooth edges make painless puncture
- Needle Gauge: 21G, 22G, 23G, 25G
- Needle Length: 3/4", 1"
- Color coded wings for gauge identification
- Sterile EO, individual pack



Safety Blood Collection Needle
Aiguille de prélèvement Sécurité

HSE0516

- Safety Type, avoid second use and injuries
- Auto-retractable needle, self-destroy holder
- Adapt to inpatient, outpatient, emergency case, outdoor injure or long distance blood collected
- Needle Gauge: 21G, 22G, 23G
- Needle Length: 1", 1 1/4", 1 1/2"
- Sterile EO, individual blister pack

Blood Collection Needle Holder
Porte tube à prélèvement Holder

HSE0517

- Made from medical grade PP
- Types: Normal type with screw lock
  Safety type with auto-release lock
- Transparent or light blue color
- Size: 20X55mm
- Can match with all size vacuum tubes






Tourniquet
Turnstile réutilisable

HSE0518

- Terylene belt, high elastic, latex-free
- A-class ABS buckle, white or milky color
- Belt color: red, green, blue or customized
- Belt size: 2.5x40cm (Adult), 2.5x35cm (Child)
- Logo printing available on both Belt or Buckle
- Reusable, Individual pack in OPP bag

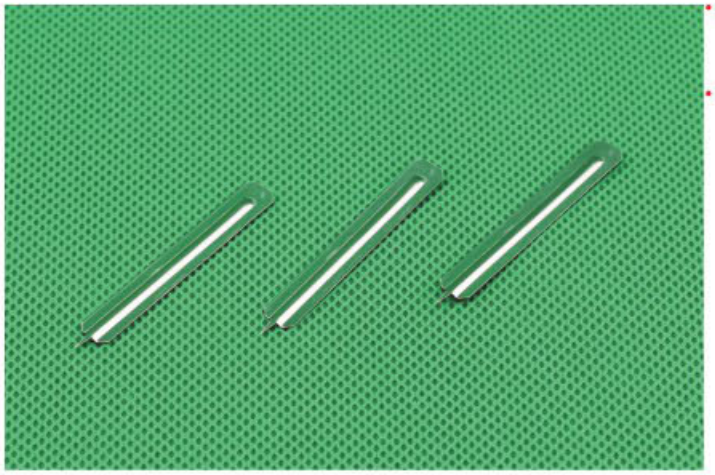

Stainless Steel Blood Lancet
Lancettes stériles boîte de 200


HSE0519


- Made from high quality stainless steel
- Sharp, smooth point, painless
- Specification: L, S
- Sterile by Gamma radiation
- Individual wrapped, box of 200pcs
- For single use only

Twist Blood Lancet
Lancettes pour stylo autopiqueur

HSE0520

- Twist type, PVC holder + stainless steel needle
- Sharp, smooth Tri-bevel point, less pain
- Fits most standard lancing devices
- Gauze: 21G, 23G, 26G, 28G, 30G
- Sterile by Gamma radiation
- Box of 100 or 200

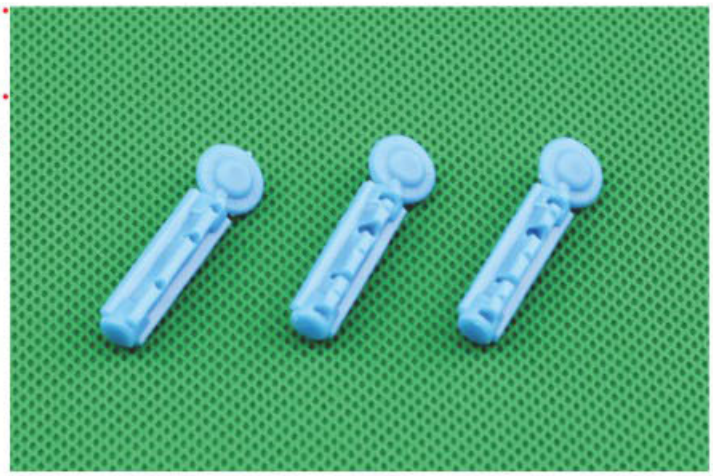


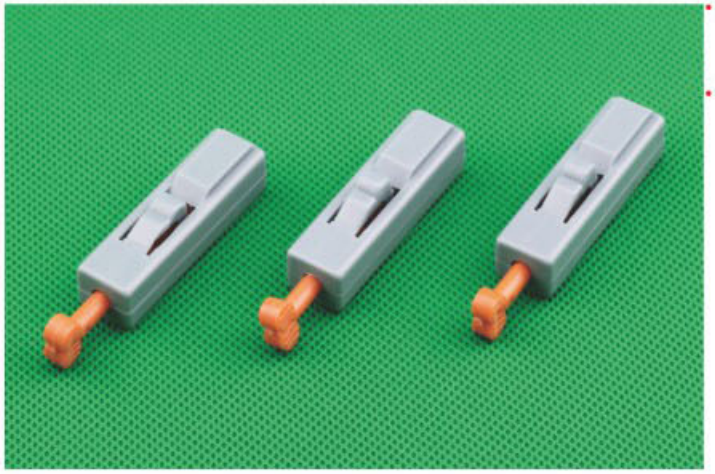

Safety Blood Lancet -Button Activated
Lancette de sécurité bouton Activé

HSE0521

- Safety type, button activated
- High quality tri-bevel needle with high-speed penetration, make painless and comfortable
- Gauze: 21G, 23G, 26G
- Sampling depth: 2.4mm
- Color coded top for gauge identification
- Sterile by Gamma radiation

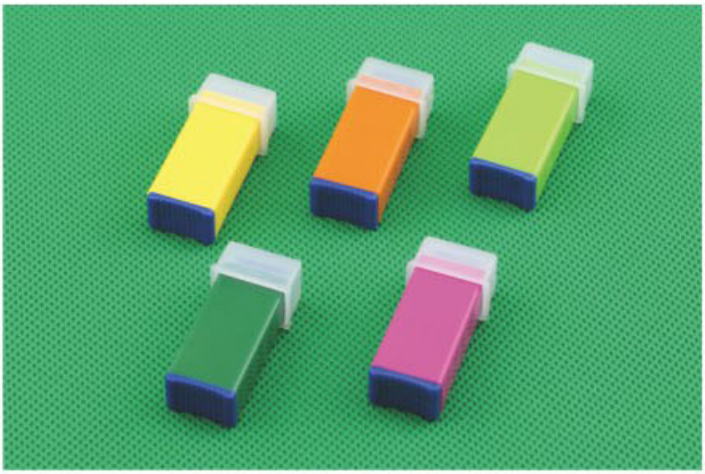

Safety Blood Lancet -Pressure Activated
Lancette de sécurité pression activé

HSE0522


- Safety type, pressure activated
- High quality tri-bevel needle with high-speed penetration, make painless and comfortable
- Gauze: 21G, 23G, 26G, 28G
- Sampling depth: 1.8mm or 2.4mm
- Color coded surface for gauge identification
- Sterile by Gamma radiation

Disposable Plastic Blood Bag
Poche à sang à usage unique

HSE0523

- Rolled or Blow-extruded PVC bag
- Single, Double, Triple or Quadruple bag
- Filled with anticoagulant solution or empty
- Anticoagulant solution: CPDA-1, CPD, SAGM
- Primary Bag capacity 150ml to 500ml
- Satellite Bag capacity 100ml to 450ml
- Plastic or Metal Donor needle 16G or 17G, Ultra-thin walled for reducing donor pain
- Sterilized by steam, non-toxic, pyrogen-free



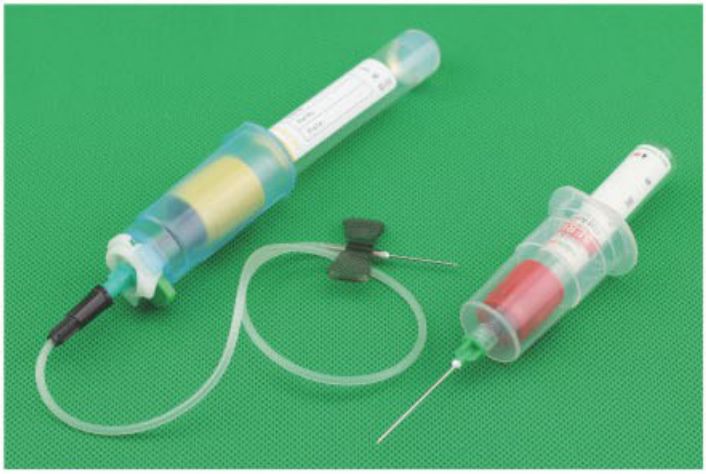

HENSO Blood Collection System
Système de collecte de sang HENSO

- One-stop solution for blood collection system
- 6 years professional manufacture & marketing expirences
- 300,000 class purifying production workshop
- Daily output up to 600,000pcs tubes and 500,000pcs needles
- Available in customized printing and packaging
- Full quality assurance with CE and ISO certify

HENSO

for better life

Quality Assurance



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in Class IIa, IIb or III)

No. G2 14 09 89326 002

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): For detail information see attachement

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex V. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class IIb and III devices an additional Annex III certificate is mandatory. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in class I in sterile conditions, sterilized systems or procedure packs)

No. G2S 14 09 89326 003

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): Sterile Urine Drainage Bag, Sterile Vaginal Speculum, Disposable Umbilical Cord Clamps, Disposable I.D. Bracelets, Disposable Dressing Kits, Disposable Gynecological Sets, Gauze Swab (Sponges), Gauze Bandages, Absorbent Cotton Rolls, Absorbent Cotton Balls, First Aid Kits, Bandages, Sterile Wound Plaster, Sterile Wound Dressing, Surgical Gowns, Face Masks, Shoe Covers, Cotton Swab (Cotton Tipped Applicators), Tongue Depressor, Sterile Feeding Tubes, Disposable Stomach Tubes, Disposable Mucus Extractors, Sterile Latex Examinative Gloves

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture in accordance with MDD Annex V. This quality assurance system covers those aspects of manufacture concerned with assuring and maintaining sterile conditions of the respective devices / device categories and conforms to the requirements of this Directive. It is subject to periodical surveillance. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex V
(Devices in class I with measuring function)

No. G2M 14 09 89326 004

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): Aneroid Sphygmomanometers

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for the manufacture in accordance with MDD Annex V. This quality assurance system covers those aspects of manufacture concerned with the metrological requirements of the respective devices / device categories and conforms to the requirements of this Directive. It is subject to periodical surveillance. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in Class IIa, IIb or III)

No. G2 14 09 89326 002

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): For detail information see attachement

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex V. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class IIb and III devices an additional Annex III certificate is mandatory. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



Attachment for Certificate No G2N 14 09 89326 001

Supplement 001 dated 2015-01-13

For the product(s)/product category (ies):

Production and Distribution of
Vacuum Blood Collection Tubes with Needles,
Disposable Blood Collection Needles,
A.V.Fistula Needles, Disposable Syringes,
Auto Disable Syringes,
Safety Syringes with Retractable Needles,
Disposable Infusion Sets,
Disposable Blood Transfusion Sets,
Scalp Vein Sets, Disposable Hypodermic Needles,
Disposable Dental Needles, Disposable IV Catheters,
Disposable Insulin Syringes,
Insulin Pen Needle, Heparin Caps,
Three-way Stopcocks (with Extension Tube),
Blood Lancet, Sterile Surgical Blade,
Disposable Scalpel with Plastic Handle,
Tracheostomy Tubes for Single Use,
Foley Catheter (Latex), Endotracheal Tubes,
Suction Connecting Tube (with and without Yankauer Handle),
Oxygen Masks, Nebulizer Masks,
Nebulizers, Venturi Masks, Nasal Oxygen Cannula,
Laryngeal Mask Airway, Silicone Urethral Catheter,
Guedel/Oropharyngeal Airway, Sterile Nelaton Catheter,
Sterile Suction Catheter, Sterile Rectal Tube,
Sterile Urine Drainage Bag, Drainage Tube,
Sterile Feeding Tubes, Disposable Stomach Tubes,
Disposable Umbilical Cord Clamps,
Disposable I.D. Bracelets,
Disposable Mucus Extractors,
Disposable Gynecologic Samplers,
Disposable Gynecological Sets,
Sterile Vaginal Specuium,

Page 2 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



Attachment for Certificate No G2N 14 09 89326 001

Supplement 001 dated 2015-01-13

Disposable Dressing Kits,
Sterile Latex Examination Gloves,
Sterile Latex Surgical Gloves,
Gauze Swab (Sponges),
Gauze Bandages, Lap Sponges,
Non-woven Sponges (with X-ray),
Sterile Paraffin Gauze Dressing, Gauze Balls,
Absorbent Gauze (Gauze in Roll, Gauze in Zigzag, Cutted Gauze),
Absorbent Cotton Rolls, Absorbent Cotton Balls,
Absorbent Zig-zag Cotton, Eye Pad,
Alcohol Swabs / Pads, First Aid Kits,
Bandages, Elastic Bandages, Crepe Cotton Bandages,
Fast Dressing Bandages(1st Aid Bandages),
Plaster of Paris Bandages, Cast Paddings,
Sterile Wound Plasters, Sterile Wound Dressing,
Zinc Oxide Adhesive Plaster,
Surgical Tapes (Non-woven, PE, Silk, Fabric),
Sports Tape (Include Kinesiology Tape, Rigid Tape and Fix Tape),
Surgical Gowns, Face Masks, Shoe Covers, Diapers,
Underpads, Surgical Towels, Surgical Drapes,
Isolation Gowns, Protective Clothings,
Non-woven caps, Medical Bed Sheets,
Cotton Swab (Cotton Tipped Applicators),
Tongue Depressor,
Digital Thermometers,
Infra-red Ear Thermometers,
Digital Blood Pressure Monitors (Digital Sphygmo-manometers),
Aneroid Sphygmomanometers, Stathoscopes
Munich, CRT3, 2015-01-14

Hans-Heiner Junker

Page 3 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany

TÜV SÜD

CE 0123

FDA

www.hensomed.com

hensomed.com

HENSO

for better life

HEADQUARTERS:

Henso Medical (Hangzhou) Co.,Ltd.
2-818 Zhongtian MCC, Tongpu Rd.,
310012 Hangzhou, China

+86 571 8604 3296 +86 571 8604 6389

HENSO (Hong Kong):

Healthaw Medical Limited
Suite 01 10/F, Carnival Commercial Building,
18 Java Road, North Point, HK

info@healthaw.com

© All rights reserved to HENSO 2018