HENSO

for better life



Diagnostic Instruments

Instruments de Diagnostic

for better life





OUR MISSION:

Since the moment of establish, Henso are committed to offer one-stop solution for medical supplies, to reduce medical expense by supply reliable products with affordable cost. We are efforts for human's better life.

GOOD MANUFACTURING PRACTICES:

Our Manufacturing plant conforms to GMP, a WHO proprietary benchmark. This standard is evident in the physical ambience of our plant, the air and water quality, manufacturing technology, packaging and the sterilization process. Ambience: Special micro and HEPA filter at all air handling units ensure minimal contamination in all manufacturing areas. Micro organism and particle concentration levels are carefully monitored by the micro-biological lab to keep these levels within safe limits. Employees undergo periodic medical checkup to maintain high standards of health and hygiene. All clean rooms are provided with a three step change room and air showers at the entrance to ensure a dust-free environment.

PURSUIT ZERO DEFECT QUALITY:

Manufacture zero-defect products is our goal of quality. We have built a series online and manual quality control measures into each stage of raw material procurement, manufacturing and packing cycle. Our Quality Control standards conform to ISO 13485:2012 and European Medical Device Directive 93/42/EEC Annex V. We also registered with US FDA. As a result, our products have been authorized to lable prestigious CE mark.

PACKING AND STERILIZATION:

Our products are packed by most modern packaging machines, to ensure minimal risk of contamination or damage during transportation. We use Ethylene Oxide to sterilize the product, as per ISO 11135/EN 550 standards, each batch were release after strict inspection.



Basal Digital Thermometer
Thermomètre basal électronique

HSM1301


- Measurement Mode: Oral, Rectal, Underarm
- Display Range: 32.0°C -42.9°C (89.6°F-109.9°F)
- Accuracy: ±0.1°C (±0.2°F)
- Response Time: 60s (available in 30s or 10s)
- Memory: last measuring reading
- LCD size: 15.5x6.5mm, 16.5x7cm, 20x7mm
- Fever alarm, Beeper alarm, Auto shut-off
- 1.5V button battery (LR/SR-41)

Flexible Digital Thermometer
Thermomètre médical flexible

HSM1302

- Soft flexible tip offer a comfortable measure
- Display Range: 32.0°C -42.9°C (89.6°F-109.9°F)
- Accuracy: ±0.1°C (±0.2°F)
- Response Time: 60s (available in 30s or 10s)
- Memory: last measuring reading
- LCD size: 15.5x6.5mm, 16.5x7cm, 20x7mm
- Fever alarm, Beeper alarm, Auto shut-off
- 1.5V button battery (LR/SR-41)



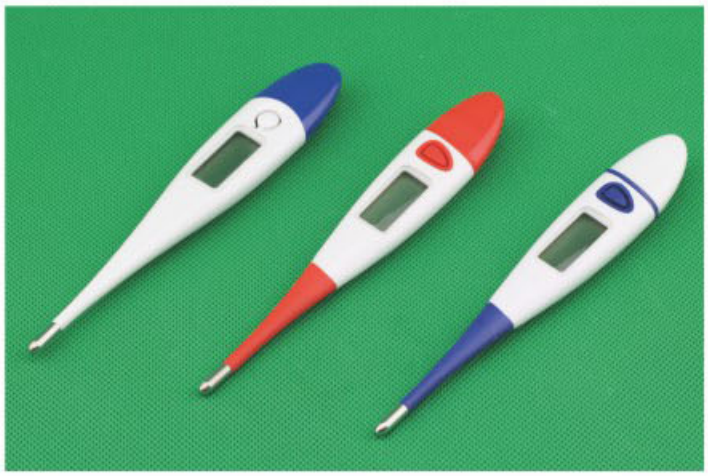

Jumbo LCD Digital Thermometer
Thermomètre médical Jumbo

HSM1303

- Large LCD display for easy reading
- Display Range: 32.0°C -42.9°C (89.6°F-109.9°F)
- Accuracy: ±0.1°C (±0.2°F)
- Response Time: 30s, 10s, 8s
- Memory: last measuring reading
- LCD Display size: 26X21mm, 31x14mm, etc.
- Fever alarm, Beeper alarm, Auto shut-off



Transparent Digital Thermometer
Thermomètre médical transparent | HSM1304

- Transparent surface
- Display Range: 32.0°C -42.9°C (89.6°F-109.9°F)
- Accuracy: ±0.1°C (±0.2°F)
- Response Time: 60s (available in 30s or 10s)
- Memory: last measuring reading
- LCD Display size: 17.5x7.5mm, 20x7mm
- Fever alarm, Beeper alarm, Auto shut-off
- 1.5V button battery (LR/SR-41)

Cartoon Digital Thermometer
Thermomètre médical enfant | HSM1305

- Cute cartoon head: Duck, Dog, Panda, Fog, etc.
- Display Range: 32.0°C -42.9°C (90.0°F-89.6°F)
- Accuracy: ±0.1°C (±0.2°F)
- Response Time: 60s (available in 30s or 10s)
- Memory: last measuring reading
- LCD size: 15.5x6.5mm, 16.5x7cm, 20x7mm
- Fever alarm, Beeper alarm, Auto shut-off
- 1.5V button battery (LR/SR-41)





Baby Pacifier Digital thermometer
Tétine thermomètre bébé | HSM1306

- Measurement Mode: oral temperature
- Display Range: 32.0°C -42.9°C (89.6°F-109.9°F)
- Accuracy: ±0.1°C (±0.2°F)
- Response Time: 2 minutes (reference only)
- Memory: last measuring reading
- LCD Display size: 15x6mm
- Fever alarm, Beeper alarm, Auto shut-off
- 1.5V button battery (LR/SR-41)



Infrared Ear Thermometer
Thermomètre auriculaire infrarouge | HSM1307

- Measurement Mode: ear temperature
- Display Range: 32.0°C -42.9°C (89.6°F-109.9°F)
- Accuracy: ±0.2°C (±0.4°F)
- Response Time: 1 second
- Memory: 10 memories
- LCD Display size: 20x16mm
- Fever alarm, Beeper alarm, Auto shut-off

4 in 1 Infrared Thermometer
Thermomètre médical infrarouge 4 en 1 | HSM1308

- 4 functions: Ear/Forehead/Ambient temperature measuring and Clock display
- Display Range: 32.0°C -42.9°C (89.6°F-109.2°F)
- Celsius and Fahrenheit (°C/°F) switchable
- Accuracy: ±0.2°C (±0.4°F)
- Response Time: 1 second
- Memory: last effective reading
- Fever alarm, Beeper alarm, Auto shut-off





Non-contact Body Infrared Thermometer
Thermomètre frontal infrarouge sans contact | HSM1309

- Non-contact Testing Forehead Temperature, Fast, Safe and Clean
- Display Range: 32.0°C -43°C (90°F-109°F)
- Accuracy: ±0.3°C (±0.54°F)
- Measuring Length: 5-15cm (2-5.9inch)
- Response Time / Laser Wavelength: 0.5 second (500ms) / 8-14)um
- 32 measuring memories
- 3 colors backlight LCD Display, for fever alarm
- Auto Shut-off after 7 seconds
- Power: 9V battery (NEDA 1604A or IEC 6LR61)
- Use Environment: Temperature:10°C -40°C (50°F -104°F);
  Relative Humidity:≤85% RH



Digital Blood Pressure Monitor -Wrist type
Tensiomètre électronique poignet

HSM1310

- Fully auto with Oscillometric method, wrist type
- Measuring Range: Pressure: (30-280)mmHg; Pulse: (40-199)Beats/Minute
- Accuracy: Pressure: ±3 mmHg; Pulse: ±5%
- Large LCD display: 29 x37mm
- Memories: 90 (single type); 60+60 (double type)
- Two 1.5V Batteries (LR03 or AAA), auto shut-off
- With WHO Indicator and Irregular Heart Rate detection

Digital Blood Pressure Monitor -Arm type
Tensiomètre électronique bras

HSM1311

- Fully Automatic Pressurization, upper arm type
- Measuring Range: Pressure: (20-300)mmHg; Pulse: (30-180)Beats/Minute
- Accuracy: Pressure: ±3 mmHg; Pulse: ±5%
- Large LCD display: 84.1 x55.1mm
- 120 Memories in 4 Groups
- Four 1.5V AA Batteries or AC adapter, auto shut-off
- Optional with WHO Classification Indicator





Digital Blood Pressure Monitor -New design
Tensiomètre électronique bras avec WHO

HSM1312

- Fully auto with Oscillometric method, upper arm type
- Measuring Range: Pressure: (30-280)mmHg; Pulse: (40-199)Beats/Minute
- Accuracy: Pressure: ±3 mmHg; Pulse: ±5%
- Large LCD display: 71 x82mm
- Memories: 90 (single type); 60+60 (double type)
- AC adapter 4x1.5V Batteries (LR6 or AA)
- With WHO Indicator and Irregular Heart Rate detection



Stethoscope
Stéthoscopes

HSM1313


- Cardiology type, for Adult or for Child
- Single head or Dual head; Aluminium, Zinc or Stainless steel material
- Chest Piece: Aluminium, Stainless steel or Cooper
- Standard Y-shape PVC tubing
- All colors available for head and PVC tubing
- Individual pack in color box

Aneroid Sphygmomanometer
Tensiomètre manobrassard

HSM1314

- Measuring Range: 0-300mmHg
- Accuracy: ±3 mmHg; Sub-division: 2mmHg
- With Aluminum Cover
- Two tubes, adult size cuff
- PVC or Latex bulb
- Color: Grey, Black, Blue or customized
- Optional with stethoscope



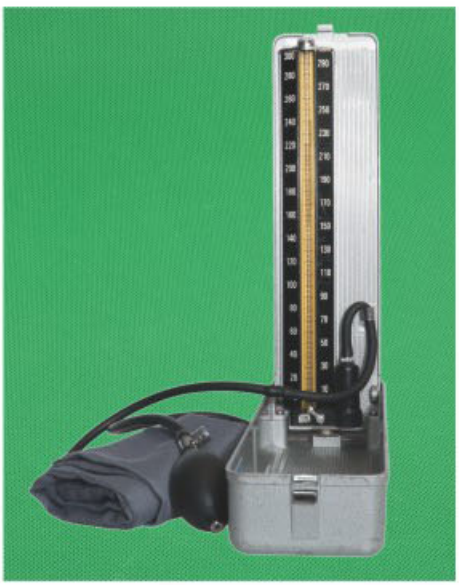

Sphygmomanometer
Tensiomètre de table à ou sans mercure

HSM1315

- Type: Mercury or Mercury-free
- Measuring Range: 0-300mmHg
- Accuracy: ±3 mmHg; Sub-division: 2mmHg
- Glass tube of excellent precision
- All metal parts are chrome-plated
- With mercury locking device
- Color: blue, grey, green, red, yellow, black
- Optional with stethoscope



Glass Clinical Thermometer
Thermomètre médical en verre

HSM1316

- Made from glass and mercury (or mercury-free)
- Style: Oral use/Rectal use/Armpit use
- Size: Small, Medium, Large
- Measuring range: 32.0°C -42°C (89.6°F-109.4°F)
- Accuracy: 0.1 in °C scale , 0.2 in °F scale
- Scale: °C or °F or °C &°F
- White or Yellow background
- Individual pack in plastic case, box of 12pcs

Browse www.infraredearthermometers.com for more Thermometers, Stethoscopes & Sphygmomanometers



HENSO

for better life

Quality Assurance



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in Class IIa, IIb or III)

No. G2 14 09 89326 002

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): For detail information see attachement

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex V. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class IIb and III devices an additional Annex III certificate is mandatory. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in class I in sterile conditions, sterilized systems or procedure packs)

No. G2S 14 09 89326 003

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): Sterile Urine Drainage Bag, Sterile Vaginal Speculum, Disposable Umbilical Cord Clamps, Disposable I.D. Bracelets, Disposable Dressing Kits, Disposable Gynecological Sets, Gauze Swab (Sponges), Gauze Bandages, Absorbent Cotton Rolls, Absorbent Cotton Balls, First Aid Kits, Bandages, Sterile Wound Plaster, Sterile Wound Dressing, Surgical Gowns, Face Masks, Shoe Covers, Cotton Swab (Cotton Tipped Applicators), Tongue Depressor, Sterile Feeding Tubes, Disposable Stomach Tubes, Disposable Mucus Extractors, Sterile Latex Examinative Gloves

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture in accordance with MDD Annex V. This quality assurance system covers those aspects of manufacture concerned with assuring and maintaining sterile conditions of the respective devices / device categories and conforms to the requirements of this Directive. It is subject to periodical surveillance. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex V
(Devices in class I with measuring function)

No. G2M 14 09 89326 004

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): Aneroid Sphygmomanometers

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for the manufacture in accordance with MDD Annex V. This quality assurance system covers those aspects of manufacture concerned with the metrological requirements of the respective devices / device categories and conforms to the requirements of this Directive. It is subject to periodical surveillance. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in Class IIa, IIb or III)

No. G2 14 09 89326 002

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): For detail information see attachement

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex V. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class IIb and III devices an additional Annex III certificate is mandatory. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



Attachment for Certificate No G2N 14 09 89326 001

Supplement 001 dated 2015-01-13

For the product(s)/product category (ies):

Production and Distribution of
Vacuum Blood Collection Tubes with Needles,
Disposable Blood Collection Needles,
A.V.Fistula Needles, Disposable Syringes,
Auto Disable Syringes,
Safety Syringes with Retractable Needles,
Disposable Infusion Sets,
Disposable Blood Transfusion Sets,
Scalp Vein Sets, Disposable Hypodermic Needles,
Disposable Dental Needles, Disposable IV Catheters,
Disposable Insulin Syringes,
Insulin Pen Needle, Heparin Caps,
Three-way Stopcocks (with Extension Tube),
Blood Lancet, Sterile Surgical Blade,
Disposable Scalpel with Plastic Handle,
Tracheostomy Tubes for Single Use,
Foley Catheter (Latex), Endotracheal Tubes,
Suction Connecting Tube (with and without Yankauer Handle),
Oxygen Masks, Nebulizer Masks,
Nebulizers, Venturi Masks, Nasal Oxygen Cannula,
Laryngeal Mask Airway, Silicone Urethral Catheter,
Guedel/Oropharyngeal Airway, Sterile Nelaton Catheter,
Sterile Suction Catheter, Sterile Rectal Tube,
Sterile Urine Drainage Bag, Drainage Tube,
Sterile Feeding Tubes, Disposable Stomach Tubes,
Disposable Umbilical Cord Clamps,
Disposable I.D. Bracelets,
Disposable Mucus Extractors,
Disposable Gynecologic Samplers,
Disposable Gynecological Sets,
Sterile Vaginal Specuium,

Page 2 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



Attachment for Certificate No G2N 14 09 89326 001

Supplement 001 dated 2015-01-13

Disposable Dressing Kits,
Sterile Latex Examination Gloves,
Sterile Latex Surgical Gloves,
Gauze Swab (Sponges),
Gauze Bandages, Lap Sponges,
Non-woven Sponges (with X-ray),
Sterile Paraffin Gauze Dressing, Gauze Balls,
Absorbent Gauze (Gauze in Roll, Gauze in Zigzag, Cutted Gauze),
Absorbent Cotton Rolls, Absorbent Cotton Balls,
Absorbent Zig-zag Cotton, Eye Pad,
Alcohol Swabs / Pads, First Aid Kits,
Bandages, Elastic Bandages, Crepe Cotton Bandages,
Fast Dressing Bandages(1st Aid Bandages),
Plaster of Paris Bandages, Cast Paddings,
Sterile Wound Plasters, Sterile Wound Dressing,
Zinc Oxide Adhesive Plaster,
Surgical Tapes (Non-woven, PE, Silk, Fabric),
Sports Tape (Include Kinesiology Tape, Rigid Tape and Fix Tape),
Surgical Gowns, Face Masks, Shoe Covers, Diapers,
Underpads, Surgical Towels, Surgical Drapes,
Isolation Gowns, Protective Clothings,
Non-woven caps, Medical Bed Sheets,
Cotton Swab (Cotton Tipped Applicators),
Tongue Depressor,
Digital Thermometers,
Infra-red Ear Thermometers,
Digital Blood Pressure Monitors (Digital Sphygmo-manometers),
Aneroid Sphygmomanometers, Stathoscopes
Munich, CRT3, 2015-01-14

Hans-Heiner Junker

Page 3 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany

TÜV SÜD

CE 0123

FDA

www.hensomed.com

hensomed.com

HENSO

for better life

HEADQUARTERS:

Henso Medical (Hangzhou) Co.,Ltd.
2-818 Zhongtian MCC, Tongpu Rd.,
310012 Hangzhou, China

+86 571 8604 3296 +86 571 8604 6389

HENSO (Hong Kong):

Healthaw Medical Limited
Suite 01 10/F, Carnival Commercial Building,
18 Java Road, North Point, HK

info@healthaw.com

© All rights reserved to HENSO 2018