HENSO

*for better life*



# Medical Catheters

# Cathéters médicaux

for better life





## OUR MISSION:

Since the moment of establish, Henso are committed to offer one-stop solution for medical supplies, to reduce medical expense by supply reliable products with affordable cost. We are efforts for human's better life.

## GOOD MANUFACTURING PRACTICES:

Our Manufacturing plant conforms to GMP, a WHO proprietary benchmark. This standard is evident in the physical ambience of our plant, the air and water quality, manufacturing technology, packaging and the sterilization process. Ambience: Special micro and HEPA filter at all air handling units ensure minimal contamination in all manufacturing areas. Micro organism and particle concentration levels are carefully monitored by the micro-biological lab to keep these levels within safe limits. Employees undergo periodic medical checkup to maintain high standards of health and hygiene. All clean rooms are provided with a three step change room and air showers at the entrance to ensure a dust-free environment.

## PURSUIT ZERO DEFECT QUALITY:

Manufacture zero-defect products is our goal of quality. We have built a series online and manual quality control measures into each stage of raw material procurement, manufacturing and packing cycle. Our Quality Control standards conform to ISO 13485:2012 and European Medical Device Directive 93/42/EEC Annex V. We also registered with US FDA. As a result, our products have been authorized to lable prestigious CE mark.

## PACKING AND STERILIZATION:

Our products are packed by most modern packaging machines, to ensure minimal risk of contamination or damage during transportation. We use Ethylene Oxide to sterilize the product, as per ISO 11135/EN 550 standards, each batch were release after strict inspection.



## Nasal Oxygen Cannula
Lunette à oxygène


**HSC0301**


- Made from soft non-toxic PVC
- Anti-crush tube in 2.1m (7ft) length
- Transparent or light green color
- Available in injection prong or dipping prong
- Size: Neonate, Child, Adult
- Sterile EO, individual pack

## Suction Catheter
Sondes d'aspiration

**HSC0302**

- Kink resistant PVC tube, X-ray line optional
- Rounded open tip with two elliptical eyes
- Connectors: Thumb finger control (cap-cone) type, T type, Plain type, Y type
- Standard length 45cm
- Color coded connector for size identification
- Size (FR): 5, 6, 8, 10, 12, 14, 16, 18, 20, 22, 24
- Sterile EO, individual pack

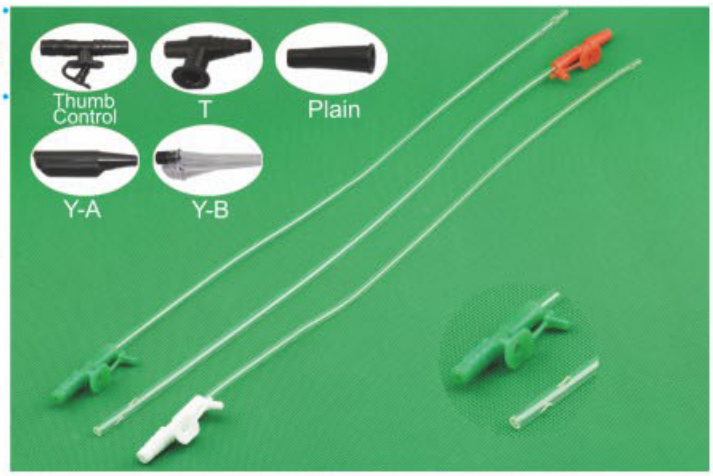
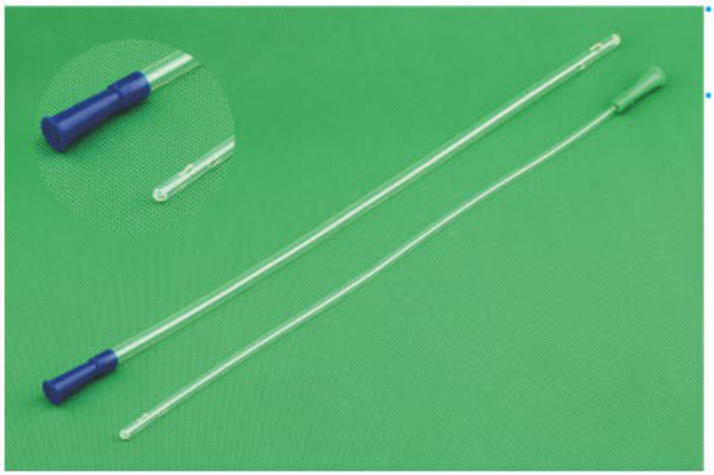
## Nelaton Catheter
Sonde vésicale Nélaton

**HSC0303**

- Made from medical grade PVC
- Standard length: 40cm
- Smooth outer surface, less pain
- Two lateral eyelet with smooth edges
- Color coded connector for size identification
- Size (FR): 6, 8, 10, 12, 14, 16, 18, 20, 22, 24
- Sterile EO, individual pack



## Stomach Tube
Sonde gastrique


**HSC0304**


- Made from PVC, non-toxic, non-pyrogenic
- Standard length: 125cm
- Soft and kink resistant PVC tube, transparent and frosted surface with graduation mark
- Four lateral eyes for efficient aspiration
- Color coded connector for size identification
- Size (FR): 6, 8, 10, 12, 14, 16, 18, 20, 22
- Sterile EO, individual pack

## Feeding Tube
Sonde à gavage

**HSC0305**

- Made from PVC, non-toxic, non-pyrogenic
- Length: 40cm (FR4-8); 120cm (FR10-22)
- Soft and kink resistant PVC tube, transparent and frosted surface with graduation mark
- Two lateral eyes allow increased flow of fluid
- Color coded connector for size identification
- Size (Fr): 4, 6, 8, 10, 12, 14, 16, 18, 20, 22
- Sterile EO, individual pack

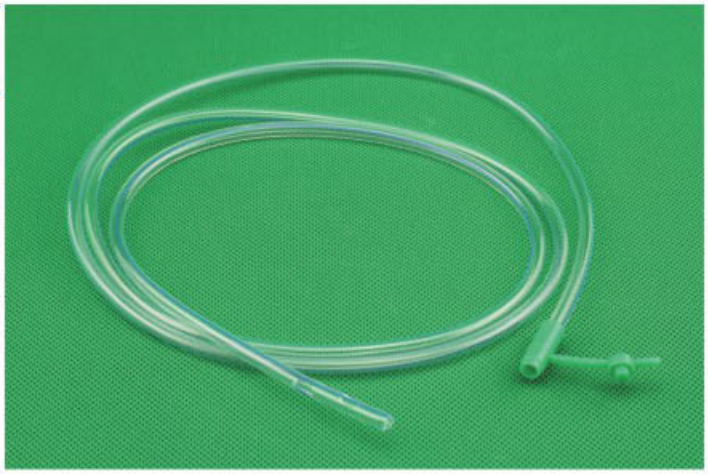


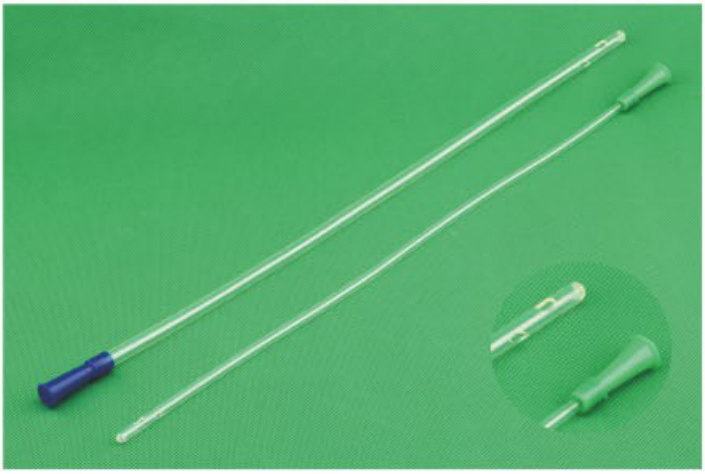

## Rectal Tube
Sondes rectales

**HSC0306**

- Made from PVC, non-toxic, non-pyrogenic
- Standard length: 38cm
- Two lateral eyelet with smooth edges
- Transparent & frosted tube with smooth surface
- Color coded connector for size identification
- Size (FR): 22, 24, 26, 28, 30, 32, 34, 36
- Sterile EO, individual pack

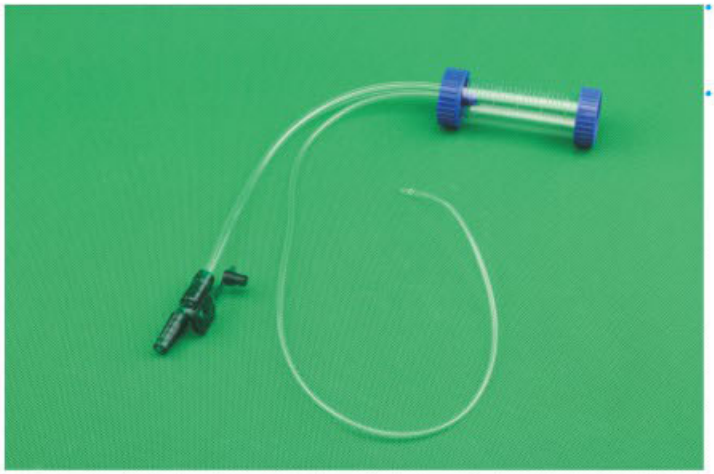

## Disposable Mucus Extractor
Extracteurs de mucus

**HSC0307**

- Made from medical grade PVC, non-toxic
- Clean transparent container with graduated volume mark
- Container volume 25ml (or 40ml)
- Soft, frosted and kink resistant PVC tubing
- Tube size 6FR-18FR
- Sterile EO, individual pack

## Enteral Feeding Bag Set
Sac d'alimentation entérale

**HSC0308**

- Rigid neck for easy filling and handing
- Plug cap or Screw cap
- Strong, dependable hanging ring
- Easy-to read graduations and easy-view translucent bag
- Bottom exit port allows complete drainage
- Pump set or Gravity set
- Bag capacity 500ml, 1000ml or 1200ml
- Sterile EO, individual pack






## Enteral Feeding Spike Set
Pointe d'alimentation entérale

**HSC0309**

- Made from medical grade PVC
- Roller Clamp, Protective Cap
- Smooth outer surface, less pain
- Y adapter available for easy flushing medications and water without disconnect set from feeding tube
- Sterile EO, individual pack

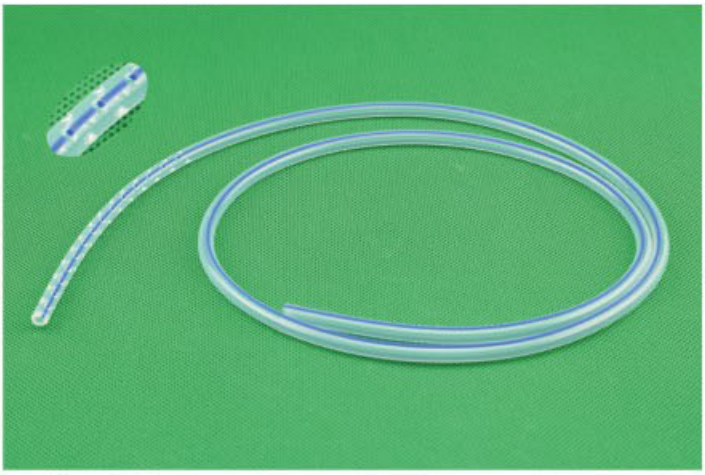

## Round Perforated Drainage Tube
Drain de Redon perforé rond

**HSC0310**


- Made from silicone or PVC
- X-ray radio opaque line throughout the tube
- Perforated on one end of tube
- It can be equipped with reservoir and trocar
- Size (FR): 10, 12, 14, 16, 18, 20
- Sterile EO, individual blister pack

## Flat Fluted Drainage Tube
Drain de Redon plat cannelé

**HSC0311**

- Made from 100% medical grade silicone
- Combine transparent round tube and white flat drain
- Full fluted design is available for optimal drainage with X-ray opaque effectiveness throughout its entire implanted segment.
- Width x Length: 8mm x 30cm, 11mm x 30cm
- Sterile EO, individual blister pack




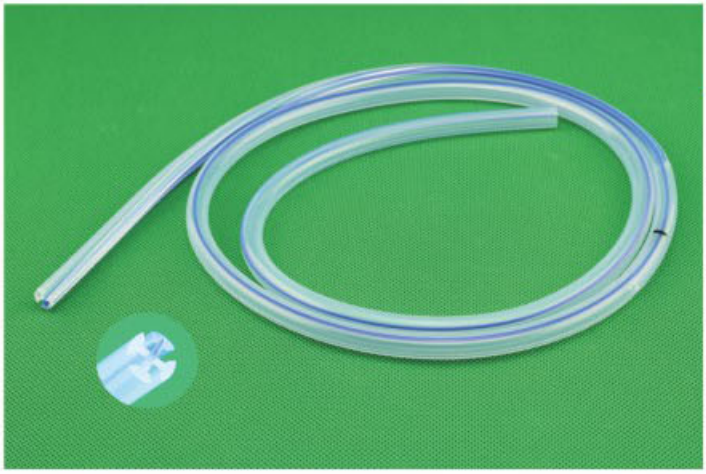

## Round Fluted Drainage Tube
Drain de Redon ronde cannelée

**HSC0312**

- Made from 100% medical grade silicone
- Four channels or fluted internal utlized to quickly remove exudates.
- X-ray radio opaque line throughout the tube
- Optional with Trocar
- Size (FR): 10, 15, 19, 24
- Used for closed wound suction draining

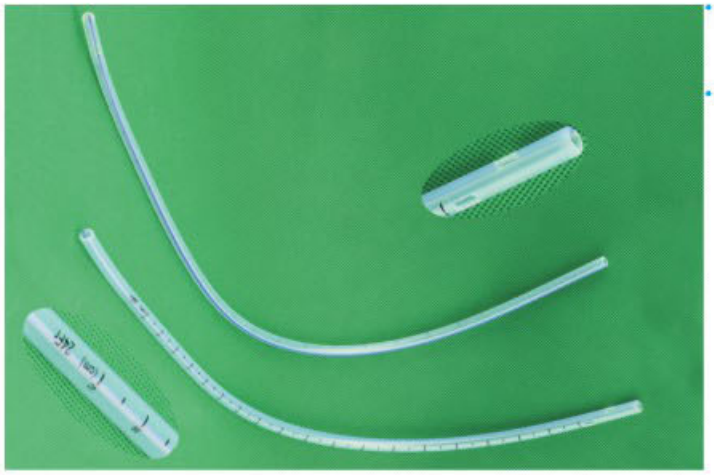

## Chest Drainage Catheter
Cathéter de Drain thoracique


**HSC0313**


- Made from medical grade PVC or Silicone
- X-ray radio opaque line throughout the tube
- Standard length 40cm with graduated mark
- Two lateral eyes with smooth surface
- With or without Trocar
- Size: 8FR-36FR
- Sterile EO, individual blister pack

## T-shaped Perforated Silicone Drain
Drain de Redon forme de T pur silicone

**HSC0314**

- Made from 100% medical grade silicone
- X-ray radio opaque line throughout the tube
- Perforated round tube design, T shape
- Size (FR): 12, 14, 16
- Sterile EO, individual blister pack

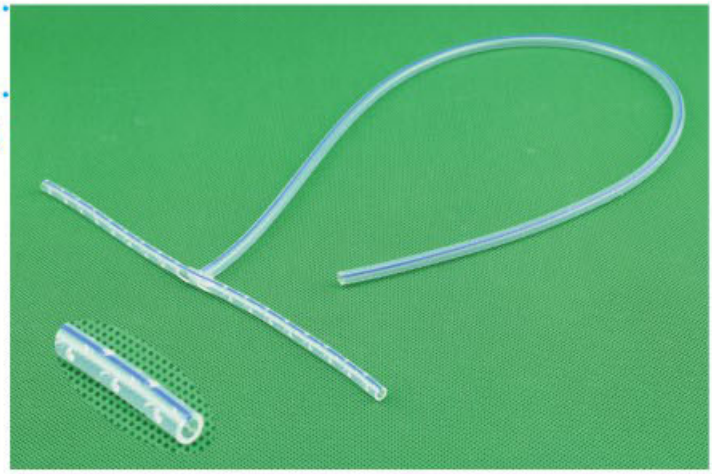

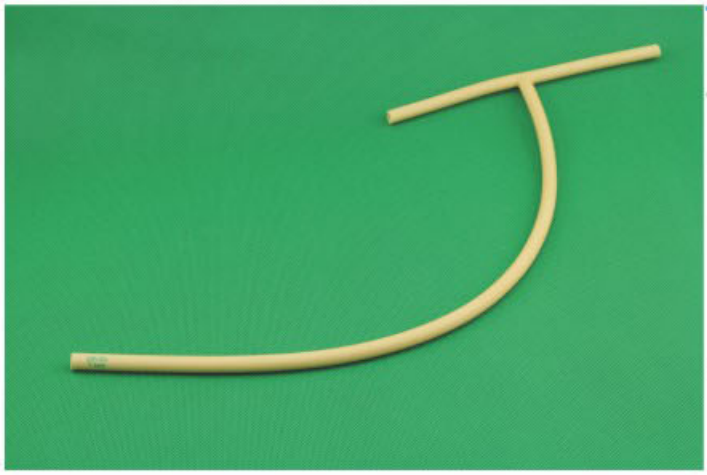

## Latex T-shape Catheter
Cathéter au latex forme de T

**HSC0315**

- Made from natural latex
- Spec.: 15x30cm and 20x40cm.
- Size: 12FR-28FR
- Sterile EO, individual blister pack
- Drainage of bile in biliary ducts

HENSO

for better life

# Quality Assurance



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in Class IIa, IIb or III)

No. G2 14 09 89326 002

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): For detail information see attachement

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex V. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class IIb and III devices an additional Annex III certificate is mandatory. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in class I in sterile conditions, sterilized systems or procedure packs)

No. G2S 14 09 89326 003

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): Sterile Urine Drainage Bag, Sterile Vaginal Speculum, Disposable Umbilical Cord Clamps, Disposable I.D. Bracelets, Disposable Dressing Kits, Disposable Gynecological Sets, Gauze Swab (Sponges), Gauze Bandages, Absorbent Cotton Rolls, Absorbent Cotton Balls, First Aid Kits, Bandages, Sterile Wound Plaster, Sterile Wound Dressing, Surgical Gowns, Face Masks, Shoe Covers, Cotton Swab (Cotton Tipped Applicators), Tongue Depressor, Sterile Feeding Tubes, Disposable Stomach Tubes, Disposable Mucus Extractors, Sterile Latex Examinative Gloves

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture in accordance with MDD Annex V. This quality assurance system covers those aspects of manufacture concerned with assuring and maintaining sterile conditions of the respective devices / device categories and conforms to the requirements of this Directive. It is subject to periodical surveillance. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices, Annex V
(Devices in class I with measuring function)

No. G2M 14 09 89326 004

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): Aneroid Sphygmomanometers

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for the manufacture in accordance with MDD Annex V. This quality assurance system covers those aspects of manufacture concerned with the metrological requirements of the respective devices / device categories and conforms to the requirements of this Directive. It is subject to periodical surveillance. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 2

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



EC Certificate

Production Quality Assurance System

Directive 93/42/EEC on Medical Devices (MDD), Annex V
(Devices in Class IIa, IIb or III)

No. G2 14 09 89326 002

Manufacturer: Henso Medical (Hangzhou) Co., Ltd.
Room 12802, 4A Cambridge Commune
No. 789 Shenhua Road
310030 Hangzhou
PEOPLE'S REPUBLIC OF CHINA

EC-Representative: Wellkang Ltd
Suite B, 29 Harley Street
LONDON
W1G 9QR
UNITED KINGDOM

Product Category(ies): For detail information see attachement

The Certification Body of TÜV SÜD Product Service GmbH declares that the aforementioned manufacturer has implemented a quality assurance system for manufacture and final inspection of the respective devices / device categories in accordance with MDD Annex V. This quality assurance system conforms to the requirements of this Directive and is subject to periodical surveillance. For marketing of class IIb and III devices an additional Annex III certificate is mandatory. See also notes overleaf.

Report No.: SH1408001
Valid from: 2015-01-13
Valid until: 2020-01-12

Date, 2015-01-14
Hans-Heiner Junker

TÜV SÜD Product Service GmbH is Notified Body with identification no. 0123

Page 1 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



Attachment for Certificate No G2N 14 09 89326 001

Supplement 001 dated 2015-01-13

For the product(s)/product category (ies):

Production and Distribution of
Vacuum Blood Collection Tubes with Needles,
Disposable Blood Collection Needles,
A.V.Fistula Needles, Disposable Syringes,
Auto Disable Syringes,
Safety Syringes with Retractable Needles,
Disposable Infusion Sets,
Disposable Blood Transfusion Sets,
Scalp Vein Sets, Disposable Hypodermic Needles,
Disposable Dental Needles, Disposable IV Catheters,
Disposable Insulin Syringes,
Insulin Pen Needle, Heparin Caps,
Three-way Stopcocks (with Extension Tube),
Blood Lancet, Sterile Surgical Blade,
Disposable Scalpel with Plastic Handle,
Tracheostomy Tubes for Single Use,
Foley Catheter (Latex), Endotracheal Tubes,
Suction Connecting Tube (with and without Yankauer Handle),
Oxygen Masks, Nebulizer Masks,
Nebulizers, Venturi Masks, Nasal Oxygen Cannula,
Laryngeal Mask Airway, Silicone Urethral Catheter,
Guedel/Oropharyngeal Airway, Sterile Nelaton Catheter,
Sterile Suction Catheter, Sterile Rectal Tube,
Sterile Urine Drainage Bag, Drainage Tube,
Sterile Feeding Tubes, Disposable Stomach Tubes,
Disposable Umbilical Cord Clamps,
Disposable I.D. Bracelets,
Disposable Mucus Extractors,
Disposable Gynecologic Samplers,
Disposable Gynecological Sets,
Sterile Vaginal Specuium,

Page 2 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany



Attachment for Certificate No G2N 14 09 89326 001

Supplement 001 dated 2015-01-13

Disposable Dressing Kits,
Sterile Latex Examination Gloves,
Sterile Latex Surgical Gloves,
Gauze Swab (Sponges),
Gauze Bandages, Lap Sponges,
Non-woven Sponges (with X-ray),
Sterile Paraffin Gauze Dressing, Gauze Balls,
Absorbent Gauze (Gauze in Roll, Gauze in Zigzag, Cutted Gauze),
Absorbent Cotton Rolls, Absorbent Cotton Balls,
Absorbent Zig-zag Cotton, Eye Pad,
Alcohol Swabs / Pads, First Aid Kits,
Bandages, Elastic Bandages, Crepe Cotton Bandages,
Fast Dressing Bandages(1st Aid Bandages),
Plaster of Paris Bandages, Cast Paddings,
Sterile Wound Plasters, Sterile Wound Dressing,
Zinc Oxide Adhesive Plaster,
Surgical Tapes (Non-woven, PE, Silk, Fabric),
Sports Tape (Include Kinesiology Tape, Rigid Tape and Fix Tape),
Surgical Gowns, Face Masks, Shoe Covers, Diapers,
Underpads, Surgical Towels, Surgical Drapes,
Isolation Gowns, Protective Clothings,
Non-woven caps, Medical Bed Sheets,
Cotton Swab (Cotton Tipped Applicators),
Tongue Depressor,
Digital Thermometers,
Infra-red Ear Thermometers,
Digital Blood Pressure Monitors (Digital Sphygmo-manometers),
Aneroid Sphygmomanometers, Stathoscopes
Munich, CRT3, 2015-01-14

Hans-Heiner Junker

Page 3 of 3

TÜV SÜD Product Service GmbH · Zertifizierstelle · Ridlerstraße 65 · 80339 München · Germany

TÜV SÜD

CE 0123

FDA

www.hensomed.com

hensomed.com

HENSO

*for better life*


HEADQUARTERS:

**Henso Medical (Hangzhou) Co.,Ltd.**
2-818 Zhongtian MCC, Tongpu Rd.,
310012 Hangzhou, China

+86 571 8604 3296 +86 571 8604 6389

HENSO (Hong Kong):

**Healthaw Medical Limited**
Suite 01 10/F, Carnival Commercial Building,
18 Java Road, North Point, HK

info@healthaw.com


© All rights reserved to HENSO 2018